

## COMPREHENSIVE SERVICES

We offer competitive repair and calibration services, as well as easily accessible documentation and free downloadable resources.

## SELL YOUR SURPLUS

We buy new, used, decommissioned, and surplus parts from every NI series. We work out the best solution to suit your individual needs.

 Sell For Cash  Get Credit  Receive a Trade-In Deal

## OBSOLETE NI HARDWARE IN STOCK & READY TO SHIP

We stock **New**, **New Surplus**, **Refurbished**, and **Reconditioned** NI Hardware.



*Bridging the gap between the manufacturer and your legacy test system.*

 1-800-915-6216

 [www.apexwaves.com](http://www.apexwaves.com)

 [sales@apexwaves.com](mailto:sales@apexwaves.com)

*All trademarks, brands, and brand names are the property of their respective owners.*

**Request a Quote**

 **CLICK HERE**

**PXIe-4303**

# DEVICE SPECIFICATIONS

# NI PXIe-4302/4303

32 Ch, 24-bit, 5 kS/s or 51.2 kS/s Simultaneous Filtered Data Acquisition Module

Français    Deutsch    日本語    한국어    简体中文
<a href="http://ni.com/manuals">ni.com/manuals</a>

This document lists specifications for the NI PXIe-4302/4303 simultaneous filtered data acquisition module. All specifications are subject to change without notice. Visit [ni.com/manuals](http://ni.com/manuals) for the most current specifications and product documentation.



**Note** To maintain forced air cooling in the PXIe system, refer to the *Maintain Forced-Air Cooling Note to Users*.

## Terminology

---

*Maximum* and *minimum* specifications characterize the warranted performance of the instrument within the recommended calibration interval and under the stated operating conditions. These specifications are subject to production verification or guaranteed by design.

*Typical* specifications are specifications met by the majority of the instruments within the recommended calibration interval and under the stated operating conditions, based on measurements taken during production verification and/or engineering development. The performance of the instrument is not warranted.

*Supplemental* specifications describe the basic function and attributes of the instrument established by design and are not subject to production verification. They provide information that is relevant for the adequate use of the instrument that is not included in the previous definitions.

All performance specifications are *typical* unless otherwise noted. These specifications are valid within the full operating temperature range. Accuracy specifications are valid within  $\pm 5$  °C of the calibration or over the full operating range as specifically noted.

## Input Characteristics

---

Number of channels.....	32 differential analog input channels
ADC resolution.....	24 bits
Type of ADC.....	Delta-Sigma



Sampling mode .....	Simultaneous
Sample rates ( $f_s$ )	
NI PXIe-4302	
Range .....	1 S/s to 5 kS/s
Resolution .....	$\leq 181.9 \mu\text{S/s}$
NI PXIe-4303	
Range .....	1 S/s to 51.2 kS/s
Resolution .....	$\leq 181.9 \mu\text{S/s}$
Input coupling .....	DC
Input ranges (FS)	
10 V range	
Nominal .....	$\pm 10 \text{ V}$
Typical .....	$\pm 10.34 \text{ V}$
Minimum .....	$\pm 10.26 \text{ V}$
100 mV range	
Nominal .....	$\pm 100 \text{ mV}$
Typical .....	$\pm 103.4 \text{ mV}$
Minimum .....	$\pm 102.4 \text{ mV}$
Maximum working voltage (signal + common mode)	
10 V range .....	$\pm 10.4 \text{ V}$
100 mV range .....	$\pm 8.5 \text{ V}$
Input impedance	
Device powered on	
AI+ to AI GND .....	$> 1 \text{ G}\Omega$
AI- to AI GND .....	$> 1 \text{ G}\Omega$
Input bias current .....	$\pm 1.5 \text{ nA}$
CMRR (DC to 60 Hz)	
10 V range .....	85 dB
100 mV range .....	125 dB
FIFO Buffer Size .....	1,023 samples
Data transfers .....	Direct memory access (DMA), programmed I/O

## Fault Protection (Power On or Off)

---

AI $\pm$ <0..31>, AIGND .....	30 V between any two pins
PFI0 .....	30 V to DGND

# Accuracy<sup>1</sup>

Measurement Conditions	Range: 10 V	
	Gain Error (% of Reading)	Offset Error ( $\mu\text{V}$ )
Typ (23 °C $\pm$ 5 °C)	0.025	859
Max (23 °C $\pm$ 5 °C)	0.031	1262
Max (0 °C to 55 °C)	0.062	2897

Measurement Conditions	Range: 100 mV	
	Gain Error (% of Reading)	Offset Error ( $\mu\text{V}$ )
Typ (23 °C $\pm$ 5 °C)	0.032	17
Max (23 °C $\pm$ 5 °C)	0.043	29
Max (0 °C to 55 °C)	0.087	68

## Temperature Stability

Range: 10 V

Gain stability..... 8 ppm/°C

Offset stability ..... 31  $\mu\text{V}/^\circ\text{C}$

Range: 100 mV

Gain stability..... 10 ppm/°C

Offset stability ..... 0.76  $\mu\text{V}/^\circ\text{C}$

<sup>1</sup> Accuracies listed are warranted for the conditions described in the tables and for up to one year from the module external calibration.

# Input Noise

**Table 1.** Total Buffered Mode Noise

Measurement Range	$f_s = 5 \text{ kS/s}$	$f_s = 51.2 \text{ kS/s}^*$
10 V Range	$22 \mu\text{V}_{\text{rms}}$	$70 \mu\text{V}_{\text{rms}}$
100 mV Range	$1 \mu\text{V}_{\text{rms}}$	$3.2 \mu\text{V}_{\text{rms}}$
*NI PXIe-4303 only.		

**Table 2.** Optional Buffered Mode IIR Filtering Noise Scaling Coefficients

Filter Cut-Off Frequency	Noise Scaling Coefficient (K)
2 kHz	1.1
1 kHz	1.8
200 Hz	3
20 Hz	12
2 Hz	30

Buffered mode noise with IIR filters

$$\text{Input Noise} = \frac{\text{Total Buffer Mode Noise}}{\sqrt{\text{Highest\_Rate} \times \frac{\text{Hz}}{\text{S/s}} \times 0.45}} \times \sqrt{K \times \text{Filter\_Cut-off\_Frequency}}$$

Example

When using the 10 V range, the buffer mode noise of the NI PXIe-4303 with the 1 kHz optional IIR filter is:

Highest\_Rate of the NI PXIe-4303 = 51.2 kS/s

Total\_Buffer\_Mode\_Noise =  $70 \mu\text{V}_{\text{rms}}$

Noise Scaling Coefficient (K) of 1 kHz filter = 1.8

$K \times \text{Filter\_Cut-off\_Frequency} = 1.8 \times 1 \text{ kHz} = 1.8 \text{ kHz}$

$$\begin{aligned} \text{Input Noise} &= \frac{\text{Total Buffer Mode Noise}}{\sqrt{\text{Highest\_Rate} \times \frac{\text{Hz}}{\text{S/s}} \times 0.45}} \times \sqrt{K \times \text{Filter\_Cut-off\_Frequency}} \\ &= \frac{70 \mu\text{V}_{\text{rms}}}{\sqrt{51.2 \text{ kS/s} \times \frac{\text{Hz}}{\text{S/s}} \times 0.45}} \times \sqrt{1.8 \text{ kHz}} = 19.6 \mu\text{V}_{\text{rms}} \end{aligned}$$

# Absolute Accuracy

---

$$\text{Absolute Accuracy} = \text{Reading} \times \text{Gain Error} + \text{Offset Error} + \text{Noise Uncertainty}$$

$$\text{Noise Uncertainty} = 3 \times \frac{\text{Random Noise}}{\sqrt{\# \text{ Samples}}}$$

where

*Random Noise* is the input noise for the sample rate used.

3 converts the RMS value to peak value for a coverage of  $3\sigma$ .

*# Samples* is the number of samples averaged

For example, when using an operating temperature of  $23\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$  with the 10 V range, the absolute accuracy at full-scale input with 5000 samples acquired at 5 kS/s is:

$$\text{Gain Error} = 0.031\% \text{ of Reading}$$

$$\text{Offset Error} = 1262\text{ }\mu\text{V}$$

$$\text{Noise Uncertainty} = \frac{22\text{ }\mu\text{V} \times 3}{\sqrt{5000}} = 0.9\text{ }\mu\text{V}$$

$$\text{Absolute Accuracy} = 10\text{ V} \times \text{Gain Error} + \text{Offset Error} + \text{Noise Uncertainty} = 4362\text{ }\mu\text{V}$$

## Phase linearity

NI PXIe-4302

( $f_{\text{in}} = \text{DC to } 2.25\text{ kHz}$ ).....  $\pm 1^{\circ}$

NI PXIe-4303

( $f_{\text{in}} = \text{DC to } 23.04\text{ kHz}$ ).....  $\pm 1^{\circ}$

## Spurious free dynamic range (SFDR)

1 kHz, -60 dBFS ..... 120 dB

## Total harmonic distortion (THD)

10 V range

1 kHz, -1 dBFS ..... -98 dB

100 mV range

1 kHz, -1 dBFS ..... -98 dB

## Crosstalk

1 kHz..... -95 dB

10 kHz..... -75 dB (NI PXIe-4303 only)

# Bandwidth and Alias Rejection

## Passband

Frequency (for  $1 \text{ S/s} \leq f_s < 25 \text{ S/s}$ )..... $\leq 0.1 \times f_s$

Frequency (for  $25 \text{ S/s} \leq f_s \leq 25.6 \text{ kS/s}$ )..... $\leq 0.45 \times f_s$

**Table 3.** In Band Flatness

Measurement Range	$f_{in} = \text{DC to 2.25 kHz}$	$f_{in} = 2.25 \text{ kHz to 23.04 kHz}^*$
10 V Range	10 mdB max	100 mdB max
100 mV Range	30 mdB max	300 mdB max
*NI PXIe-4303 only.		

## Stopband

Frequency (for  $1 \text{ S/s} \leq f_s < 25 \text{ S/s}$ )..... $\leq 0.9 \times f_s$

Frequency (for  $25 \text{ S/s} \leq f_s \leq 25.6 \text{ kS/s}$ )..... $\leq 0.57 \times f_s$

Rejection ..... 100 dB

## Alias-free bandwidth

(for  $1 \text{ S/s} \leq f_s < 25 \text{ S/s}$ ).....  $0.1 \times f_s$

## Alias-free bandwidth

(for  $25 \text{ S/s} \leq f_s \leq 25.6 \text{ kS/s}$ ).....  $0.45 \times f_s$

## Minimum frequency

for ADC alias hole ..... 3.320313 MHz

Rejection at alias hole ..... 100 dB

## Uncompensated filter delay<sup>1</sup>

$$\text{Group Delay} = \text{Analog Delay} + \text{Digital Filter Group Delay}^2$$

### Analog delay

10 V range..... 6.77  $\mu\text{s}$

100 mV range..... 7.76  $\mu\text{s}$

<sup>1</sup> The compensated digital filter group delay is a result of using the anti-alias filtering in buffered mode. Hardware automatically compensates for this group delay when synchronizing. Hardware does not compensate for filter delay from either the analog filter or the optional buffered mode digital filter or the filter used for hardware-timed single point mode.

<sup>2</sup> Digital filter group delay results from using the optional IIR filter in buffered mode or the IIR filter selected in hardware-timed single point mode.

Compensated digital filter group delay ..... 1.79742 ms + Variable Filter Delay

Sample Rate	Variable Filter Delay (Samples)
$1 \text{ S/s} \leq f_s < 25 \text{ S/s}$	4.000
$25.0 \text{ S/s} \leq f_s \leq 25.3 \text{ S/s}$	57.995
$25.3 \text{ S/s} < f_s \leq 50.7 \text{ S/s}$	57.991
$50.7 \text{ S/s} < f_s \leq 101.3 \text{ S/s}$	57.981
$101.3 \text{ S/s} < f_s \leq 202.7 \text{ S/s}$	57.963
$202.7 \text{ S/s} < f_s \leq 405.3 \text{ S/s}$	57.926
$405.3 \text{ S/s} < f_s \leq 810.6 \text{ S/s}$	57.852
$810.6 \text{ S/s} < f_s \leq 1621.2 \text{ S/s}$	57.703
$1621.2 \text{ S/s} < f_s \leq 3242.5 \text{ S/s}$	57.406
$3242.5 \text{ S/s} < f_s \leq 6485.0 \text{ S/s}$	56.813
$6485.0 \text{ S/s} < f_s \leq 12970.0 \text{ S/s}$	55.625
$12970.0 \text{ S/s} < f_s \leq 25939.9 \text{ S/s}$	53.250
$25939.9 \text{ S/s} < f_s \leq 51200 \text{ S/s}$	48.500

## Channel to Channel Matching<sup>1</sup>

**Table 4.** Gain Matching

Measurement Range	Input Signal Frequency ( $f_{in}$ )	
	DC to 2.25 kHz	2.25 kHz to 23.04 kHz*
10 V Range	17 mdB max	170 mdB max
100 mV Range	34 mdB max	340 mdB max

\* NI PXIe-4303 only.

Phase matching

$$10 \text{ V range} \dots\dots\dots \frac{0.035^\circ}{\text{kHz}} \times f_{in}$$

$$100 \text{ mV range} \dots\dots\dots \frac{0.045^\circ}{\text{kHz}} \times f_{in}$$


<sup>1</sup> Identical channel configurations.




# Optional Buffered Mode IIR Filtering

Filter Cut-Off Frequency	Filter Type	Stopband Attenuation	Passband Ripple
2 kHz Filter	Fourth order, Elliptic Filter	-120 dB	0.2 dB
1 kHz Filter	Fourth order, Elliptic Filter	-120 dB	0.2 dB
200 Hz Filter	Fourth order, Elliptic Filter	-120 dB	0.2 dB
20 Hz Filter	Fourth order, Elliptic Filter	-120 dB	0.2 dB
2 Hz Filter	Fourth order, Elliptic Filter	-120 dB	0.2 dB


**Figure 1. Magnitude Response**

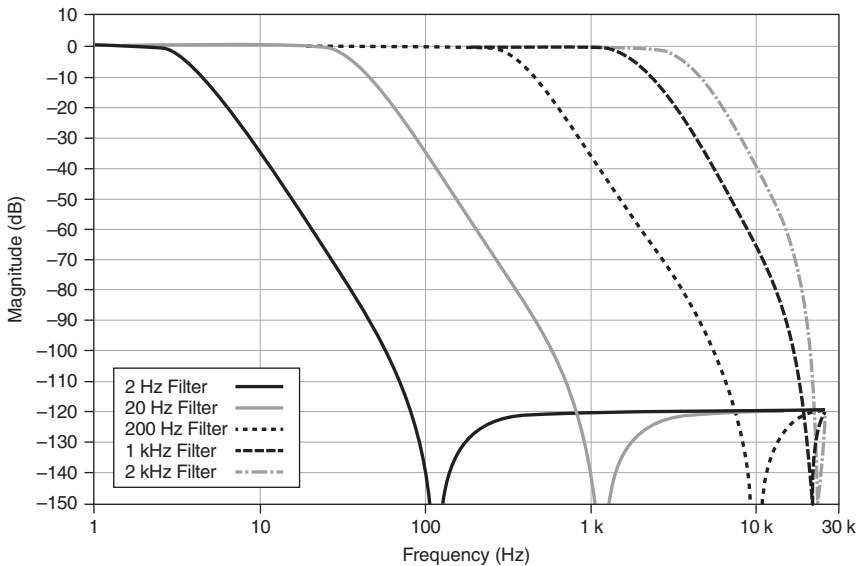


**Figure 2. Passband**

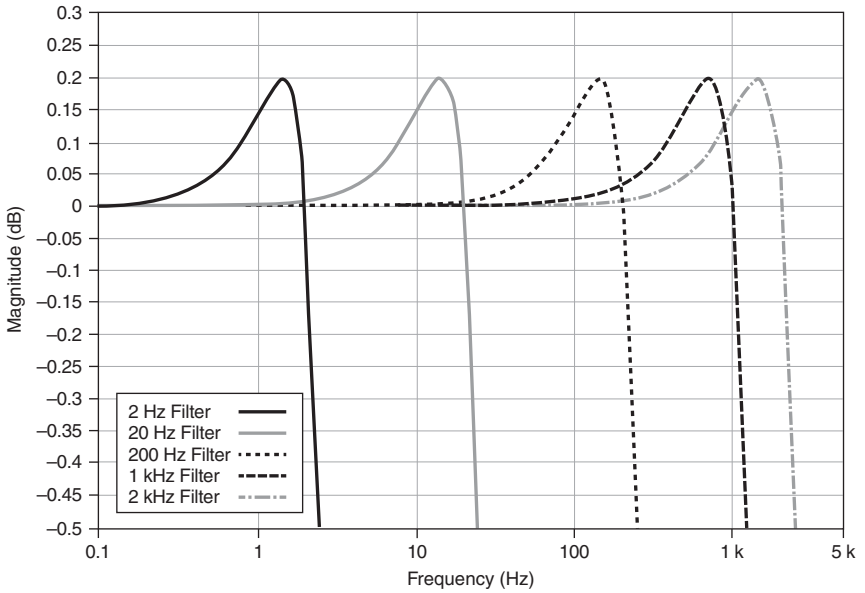

**Figure 3. Phase Response**

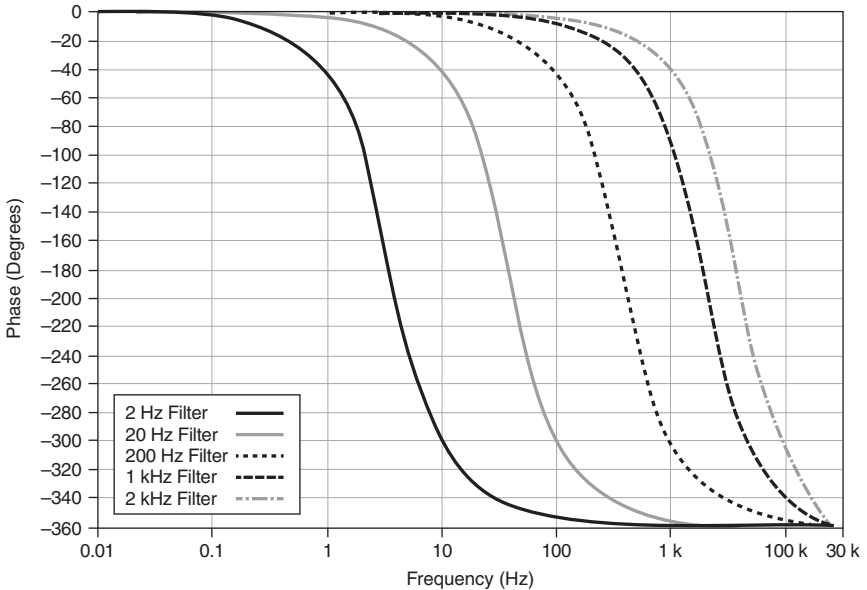

**Figure 4. Group Delay**

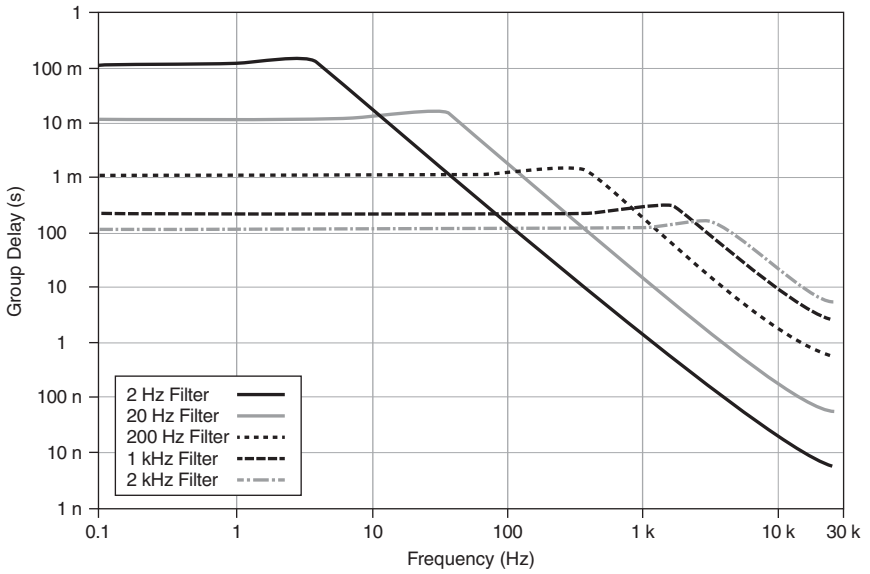

**Table 5. Digital Filter Group Delay**

Filter Cut-Off Frequency	Group Delay at 0.1 Hz
2 kHz Filter	113.4 μs
1 kHz Filter	227.4 μs
200 Hz Filter	1.1385 ms
20 Hz Filter	11.3856 ms
2 Hz Filter	113.856 ms

# Hardware-Timed Single Point Sample Mode

## Acquisition rate<sup>1</sup>

Minimum .....	1 S/s
Maximum	
NI PXIe-4302 .....	5 kS/s
NI PXIe-4303 .....	51.2 kS/s

**Table 6.** Measured Hardware-Timed Single Point Sample Mode Noise at 23 °C


Filter Cut-Off Frequency	10 V Range	100 mV Range
3 kHz Filter	31.8 $\mu\text{V}_{\text{rms}}$	1.0 $\mu\text{V}_{\text{rms}}$
2 kHz Filter	29.7 $\mu\text{V}_{\text{rms}}$	906 nV <sub>rms</sub>
1 kHz Filter	27.2 $\mu\text{V}_{\text{rms}}$	661 nV <sub>rms</sub>
500 Hz Filter	25.6 $\mu\text{V}_{\text{rms}}$	492 nV <sub>rms</sub>
200 Hz Filter	24.7 $\mu\text{V}_{\text{rms}}$	357 nV <sub>rms</sub>
100 Hz Filter	24.6 $\mu\text{V}_{\text{rms}}$	300 nV <sub>rms</sub>

## Hardware-Timed Single Point Filtering


Filter type .....	Fourth order, elliptic filter
Stopband attenuation .....	-120 dB
Passband ripple .....	0.2 dB

<sup>1</sup> Depends on the system setup and application time. Refer to the *NI PXIe-4302/4303 User Manual* for more information.


**Figure 5. Filter Magnitude Response**

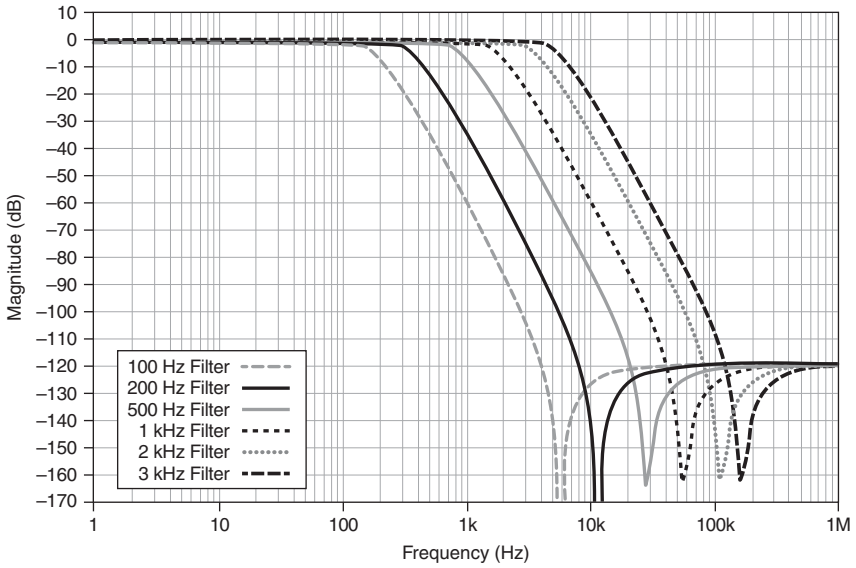


**Figure 6. Passband Ripple**

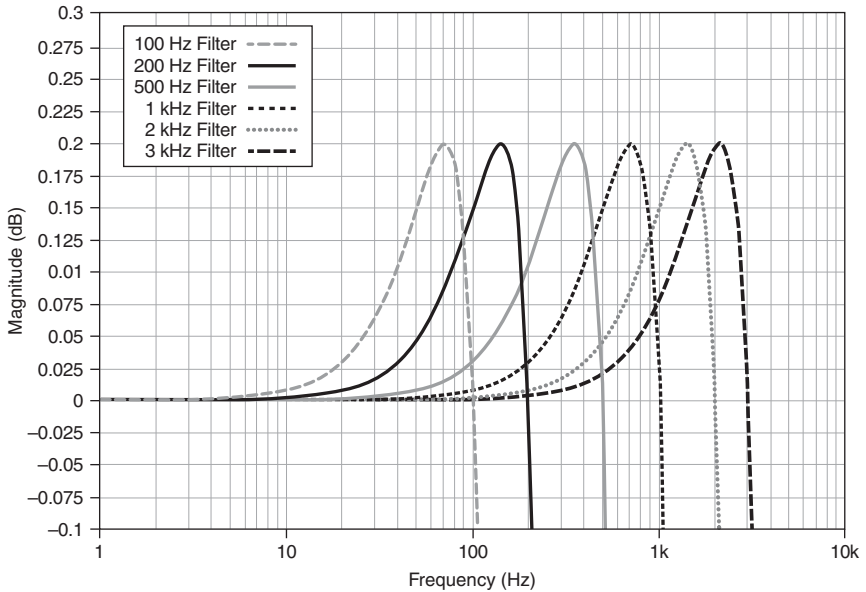

**Figure 7. Filter Phase Response**

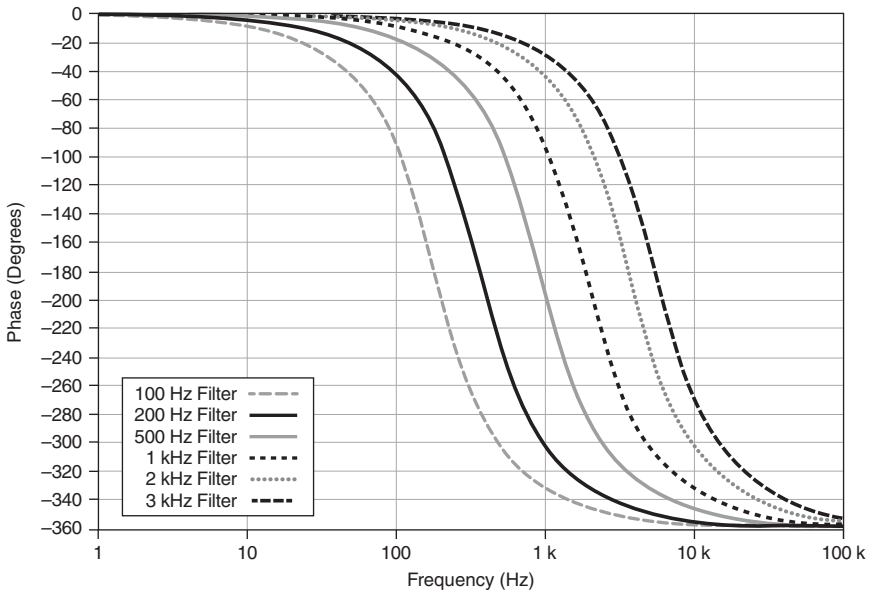

**Figure 8. Filter Group Delay**

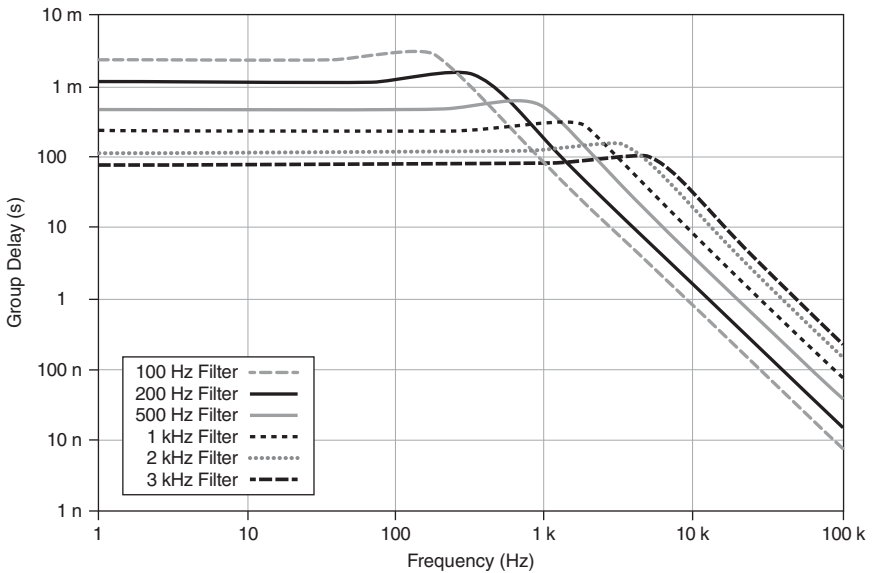

**Table 7. Digital Filter Group Delay**

<b>Filter Cut-Off Frequency</b>	<b>Group Delay at 1 Hz</b>
3 kHz Filter	75.9 $\mu$ s
2 kHz Filter	113.9 $\mu$ s
1 kHz Filter	227.7 $\mu$ s
500 Hz Filter	455.4 $\mu$ s
200 Hz Filter	1.1386 ms
100 Hz Filter	2.28 ms

Hardware-timed single point ADC group delay<sup>1</sup> ..... 1.6  $\mu$ s

## Internal Frequency Timebase Characteristics

---

Frequency..... 106.25 MHz  
 Accuracy .....  $\pm$ 50 ppm

## Synchronization

---

Reference clock source ..... Onboard 106.25 MHz clock,  
 Backplane PXIe\_CLK100

## Task Resources<sup>2</sup>

---

Timing engines..... 4  
 Buffered mode streams ..... 4  
 Hardware-timed single point streams ..... 4  
 Maximum channels per stream ..... 8

<sup>1</sup> When in hardware-timed single point mode, *Total group delay = ADC group delay + Filter group delay.*

<sup>2</sup> The NI PXIe-4302/4303 can operate four independent timing engines simultaneously. Each timing engine can utilize one or more buffered mode or hardware-timed single point streams, but not both types simultaneously. Refer to the *NI PXIe-4302/4303 User Manual* for more details about timing engines and DSP streams.

# Triggers

---

## Analog trigger

Purpose .....	Reference trigger only
Source .....	AI<0..31>
Level .....	Full scale (depending on input range), programmable
Mode .....	Rising-edge, Rising-edge with hysteresis, Falling-edge, Falling-edge with hysteresis, Entering Window, Leaving Window
Resolution .....	24 bits

## Digital trigger

Purpose .....	Start or reference trigger
Source .....	PFI0, PXI_TRIG <0..7>, PXI_STAR, PXIe_DSTAR <A..B>
Polarity .....	Software-selectable
Minimum pulse width .....	100 ns for PXI_TRIG <0..7>, 20 ns for others

# Output Timing Signals

---

Sources .....	Sample Clock, Start Trigger Out, Reference Trigger Out
Destinations .....	PFI0, PXI_TRIG <0..7>, PXIe_DSTARC
Polarity .....	Software-selectable

# PFI Characteristics

---

## Input

Logic compatibility .....	3.3 V to 5 V
High, $V_{IH}$ .....	2.40 V
Low, $V_{IL}$ .....	0.95 V
Input impedance .....	10 k $\Omega$

## Output

High, $V_{OH}$ .....	3.43 V max
Sourcing 5 mA .....	2.88 V min
Low, $V_{OL}$ sinking 5 mA .....	0.33 V max
Output impedance .....	50 $\Omega$
Output current .....	$\pm 5$ mA min



# Bus Interface

---

Form factor .....	x1 PXI Express peripheral module, Specification rev 1.0 compliant
Slot compatibility .....	PXI Express or PXI Express hybrid slots
DMA channels .....	4, analog input

# Calibration

---

You can obtain the calibration certificate and information about calibration services for the NI PXIe-4302/4303 at [ni.com/calibration](http://ni.com/calibration).

Recommended warm-up time .....	15 minutes
Calibration interval .....	1 year

# Power Requirement

---

+12 V .....	1.3 A
+3.3 V .....	1.1 A

# Physical Requirements

---

Dimensions .....	Standard 3U PXIe, 16 cm × 10 cm (6.3 in. × 3.9 in.)
Weight .....	156 g (5.5 oz)
I/O connector .....	96-pin male DIN 41612/IEC 60603-2 connector



**Caution** Clean the hardware with a soft, nonmetallic brush. Make sure that the hardware is completely dry and free from contaminants before returning it to service.

# Environmental Specifications

---

Maximum altitude .....	2,000 m (800 mbar)
Pollution Degree .....	2
Indoor use only.	

## Operating Environment

Ambient temperature range .....	0 °C to 55 °C (Tested in accordance with IEC 60068-2-1 and IEC 60068-2-2. Meets MIL-PRF-28800F Class 3 low temperature limit and MIL-PRF-28800F Class 2 high temperature limit.)
Relative humidity range.....	10% to 90%, noncondensing (Tested in accordance with IEC 60068-2-56.)

## Storage Environment

Ambient temperature range .....	-40 °C to 71 °C (Tested in accordance with IEC 60068-2-1 and IEC 60068-2-2. Meets MIL-PRF-28800F Class 3 limits.)
Relative humidity range.....	5% to 95%, noncondensing (Tested in accordance with IEC 60068-2-56.)

## Shock and Vibration

---

Operating shock.....	30 g peak, half-sine, 11 ms pulse (Tested in accordance with IEC 60068-2-27. Meets MIL-PRF-28800F Class 2 limits.)
Random vibration	
Operating .....	5 Hz to 500 Hz, 0.3 g <sub>rms</sub>
Non-operating.....	5 Hz to 500 Hz, 2.4 g <sub>rms</sub> (Tested in accordance with IEC 60068-2-64. Non-operating test profile exceeds the requirements of MIL-PRF-28800F, Class 3.)

## Safety

---

This product meets the requirements of the following standards of safety for electrical equipment for measurement, control, and laboratory use:

- IEC 61010-1, EN 61010-1
- UL 61010-1, CSA 61010-1



**Note** For UL and other safety certifications, refer to the product label or the [Online Product Certification](#) section.



**Caution** The protection provided by the NI PXIe-4302/4303 can be impaired if it is used in a manner not described in this documents.

# Electromagnetic Compatibility

---

This product meets the requirements of the following EMC standards for electrical equipment for measurement, control, and laboratory use:

- EN 61326-1 (IEC 61326-1): Class A emissions; Basic immunity
- EN 55011 (CISPR 11): Group 1, Class A emissions
- EN 55022 (CISPR 22): Class A emissions
- EN 55024 (CISPR 24): Immunity
- AS/NZS CISPR 11: Group 1, Class A emissions
- AS/NZS CISPR 22: Class A emissions
- FCC 47 CFR Part 15B: Class A emissions
- ICES-001: Class A emissions



**Note** In the United States (per FCC 47 CFR), Class A equipment is intended for use in commercial, light-industrial, and heavy-industrial locations. In Europe, Canada, Australia and New Zealand (per CISPR 11) Class A equipment is intended for use only in heavy-industrial locations.



**Note** Group 1 equipment (per CISPR 11) is any industrial, scientific, or medical equipment that does not intentionally generate radio frequency energy for the treatment of material or inspection/analysis purposes.



**Note** For EMC declarations and certifications, and additional information, refer to the [Online Product Certification](#) section.

## CE Compliance

---

This product meets the essential requirements of applicable European Directives as follows:

- 2014/35/EU; Low-Voltage Directive (safety)
- 2014/30/EU; Electromagnetic Compatibility Directive (EMC)

## Online Product Certification

---

Refer to the product Declaration of Conformity (DoC) for additional regulatory compliance information. To obtain product certifications and the DoC for this product, visit [ni.com/certification](http://ni.com/certification), search by model number or product line, and click the appropriate link in the Certification column.

# Environmental Management

---

NI is committed to designing and manufacturing products in an environmentally responsible manner. NI recognizes that eliminating certain hazardous substances from our products is beneficial to the environment and to NI customers.

For additional environmental information, refer to the *Minimize Our Environmental Impact* web page at [ni.com/environment](http://ni.com/environment). This page contains the environmental regulations and directives with which NI complies, as well as other environmental information not included in this document.

## Waste Electrical and Electronic Equipment (WEEE)



**EU Customers** At the end of the product life cycle, all products *must* be sent to a WEEE recycling center. For more information about WEEE recycling centers, National Instruments WEEE initiatives, and compliance with WEEE Directive 2002/96/EC on Waste and Electronic Equipment, visit [ni.com/environment/weee](http://ni.com/environment/weee).

## 电子信息产品污染控制管理办法（中国 RoHS）



**中国客户** National Instruments 符合中国电子信息产品中限制使用某些有害物质指令 (RoHS)。关于 National Instruments 中国 RoHS 合规性信息，请登录 [ni.com/environment/rohs\\_china](http://ni.com/environment/rohs_china)。(For information about China RoHS compliance, go to [ni.com/environment/rohs\\_china](http://ni.com/environment/rohs_china).)

## World Wide Support and Services

---

The National Instruments website is your complete resource for technical support. At [ni.com/support](http://ni.com/support) you have access to everything from troubleshooting and application development self-help resources to email and phone assistance from NI Application Engineers.

Visit [ni.com/services](http://ni.com/services) for NI Factory Installation Services, repairs, extended warranty, and other services.

Visit [ni.com/register](http://ni.com/register) to register your National Instruments product. Product registration facilitates technical support and ensures that you receive important information updates from NI.

National Instruments corporate headquarters is located at 11500 North Mopac Expressway, Austin, Texas, 78759-3504. National Instruments also has offices located around the world. For telephone support in the United States, create your service request at [ni.com/support](http://ni.com/support) or dial 1 866 ASK MYNI (275 6964). For telephone support outside the United States, visit the Worldwide Offices section of [ni.com/niglobal](http://ni.com/niglobal) to access the branch office websites, which provide up-to-date contact information, support phone numbers, email addresses, and current events.

Refer to the *NI Trademarks and Logo Guidelines* at [ni.com/trademarks](http://ni.com/trademarks) for more information on NI trademarks. Other product and company names mentioned herein are trademarks or trade names of their respective companies. For patents covering NI products/technology, refer to the appropriate location: **Help»Patents** in your software, the `patents.txt` file on your media, or the *National Instruments Patents Notice* at [ni.com/patents](http://ni.com/patents). You can find information about end-user license agreements (EULAs) and third-party legal notices in the `readme` file for your NI product. Refer to the *Export Compliance Information* at [ni.com/legal/export-compliance](http://ni.com/legal/export-compliance) for the NI global trade compliance policy and how to obtain relevant HTS codes, ECCNs, and other import/export data. NI MAKES NO EXPRESS OR IMPLIED WARRANTIES AS TO THE ACCURACY OF THE INFORMATION CONTAINED HEREIN AND SHALL NOT BE LIABLE FOR ANY ERRORS. U.S. Government Customers: The data contained in this manual was developed at private expense and is subject to the applicable limited rights and restricted data rights as set forth in FAR 52.227-14, DFAR 252.227-7014, and DFAR 252.227-7015.

© 2015–2016 National Instruments. All rights reserved.